
	<b>ANALYSENZERTIFIKAT CERTIFICATE OF ANALYSIS</b>	DQ1P00AZ.02
---	---	-------------

### Coagulation Control N 5x1ml

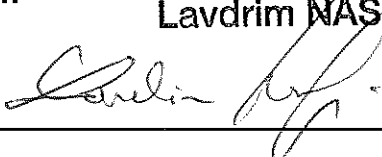
REF      5020040  
LOT      1P14B00.04  
      30-Jun-2016

<b>Analytische Prozedur Analytical Procedure</b>		<b>Anforderung Requirement</b>	<b>Ergebnis Result</b>	
pH		7.4 – 7.8	7.7	OK
Virologie Virology	HbsAg HIV 1,2 Ab HCV	Negative Negative Negative	Negative Negative Negative	OK

Verwendbarkeit Usability Ceveron <sup>®</sup> alpha	DAPTTIN TC	28.0 – 38.0 sec	33.7 sec	OK
	FVIII:C chromogenic substrate	72 – 120 %	94.9 %	OK
	Technoplastin HIS (INR)	0.88 – 1.06	1.00	OK
	Technoplastin HIS (%)	92.0 – 120.0 %	99.4 %	OK

**Durchführung von  
Prepared by**

**Lavdrim NASUFI**

  
\_\_\_\_\_

*24-Apr-2013*  
\_\_\_\_\_

Datum / Date:

**Freigabe von  
Approved by**

**Harald SEVCIK**

  
\_\_\_\_\_

*24. Apr. 2013*  
\_\_\_\_\_

Datum / Date: