
	<b>ANALYSENZERTIFIKAT</b> <b>CERTIFICATE OF ANALYSIS</b>	DQ6V0AAZ.03
---	---	-------------

### Dapttin TC 5x2mL

REF      5035060  
LOT      6V53BA0.01  
      31-May-2017

Analytische Prozedur Analytical Procedure		Anforderung Requirement	Ergebnis Result		
pH		6.6 – 7.2	6.9	OK	
Verwendbarkeit Usability Ceveron® alpha	Dapttin TC, sec	CCN <span style="border: 1px solid black; padding: 1px;">LOT</span> 1P37B00	33.1 – 40.9 sec	36.8	OK
		CCA <span style="border: 1px solid black; padding: 1px;">LOT</span> 3P38B00	96.5 – 119.1 sec	105.4	OK
Etiketten und Barcode Überprüfung Label and bar code Verification			OK		

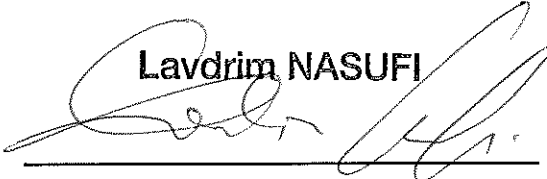
**Durchführung von**  
**Prepared by**

**Fikret NASUFI** *Fikret Nasufi*  


---

*27-May-2015*  
Datum / Date:

**Freigabe von**  
**Approved by**

  
**Lavdrim NASUFI**  


---

*27-May-2015*  
Datum / Date: