





**ANALYSENZERTIFIKAT
CERTIFICATE OF ANALYSIS**

DQ...00AZ


PAP Complex ELISA Kit 96T.

REF TC12060
LOT 120602B3.01
 28 – Feb – 2015

Inhalt Content	Reagenz Reagent	LOT	
1 x 12	PAP Plate	RGY31B0	28-FEB-2015
1 x 0.3mL	anti PAP POX	RBK21B1	30-JUN-2015
2 x 20mL	Wash buffer Concentrate	RBE31B0	30-APR-2015
1 x 20mL	Dilution Buffer	RAF31B0	30-JUN-2016
1 x 12mL	TMB Substrate	RKN32B0	31-MAY-2015
1 x 12mL	Stop solution	RKK31B0	28-FEB-2015
1 x 0,5mL	PAP-Calibrator 1	1BM11B0	31-MAR-2015
1 x 0.5mL	PAP-Calibrator 2	2BM11B0	31-MAR-2015
1 x 0.5mL	PAP-Calibrator 3	3BM11B0	31-MAR-2015
1 x 0.5mL	PAP-Calibrator 4	4BM11B0	31-MAR-2015
1 x 0.5mL	PAP-Calibrator 5	5BM11B0	31-MAR-2015
1 x 0.5mL	PAP high Control	ABM11B0	31-MAR-2015
1 x 0.5mL	PAP low Control	BBM11B0	31-MAR-2015

Analytische Prozedur Analytical Procedure		Anforderung Requirement	Ergebnis Result	
OD	Calibrator 1	OD: 1 – 2.5	1.661	OK
	Calibrator 5	OD: < 0.2	0.009	OK
Verwendbarkeit Usability	High Control (ABM11B0)	87.9 – 163.1 ng/mL	140.085	OK
	Low Control (BBM11B0)	20.6 – 48.0 ng/mL	28.892	OK

Standardgerade / standard curve:

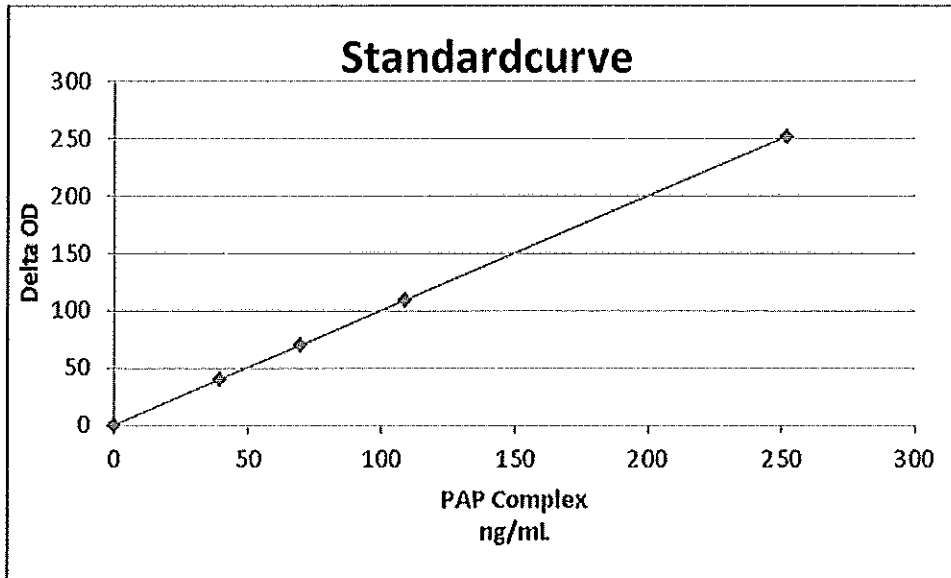

Durchführung von
Prepared by

Michael RIHA

14-Aug-2013

Datum / Date:

Freigabe von
Approved by

Harald SEVCIK

14. AUG. 2013

Datum / Date: