

# Thrombodynamics Analyser

## Thrombodynamics-4D assay



24.08.2018 14:07

Measurement title: FIX Deficiency\_2% TD4D  
 Plasma type: Fresh PFP  
 Sample code: Example PLS #3



**PLS**



Fibrin dynamics parameters	Unit	Parameter	Value	Norm.
Rate of clot growth	um/min	V	24,0	34,0-44,0
Lag time	min	Tlag	0,9	0,6-1,5
Initial rate of clot growth	um/min	Vi	45,4	59,0-69,0
Stationary rate of clot growth	um/min	Vst	24,0	34,0-44,0
Clot size at 30 min	um	CS	1040	1380-1640
Clot density	a.u.	D	18011	19500-34200
Spontaneous clotting	min	Tsp		30,0-

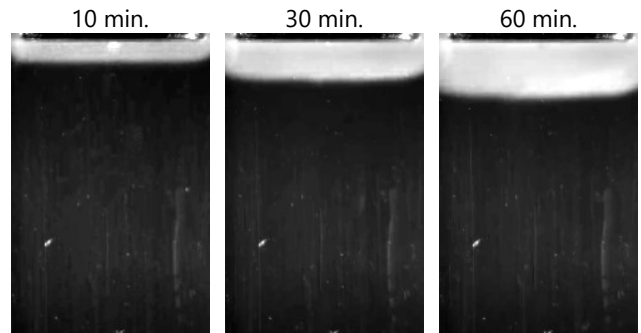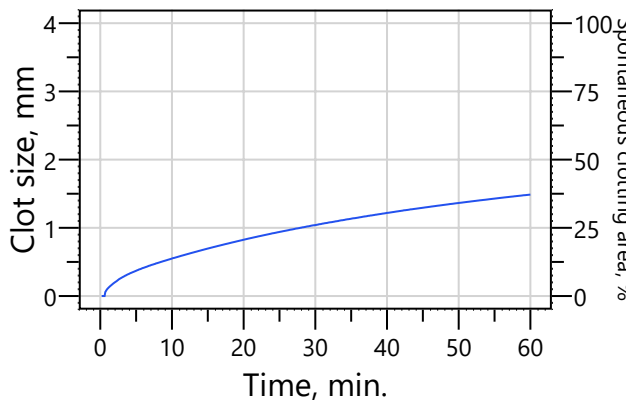

Thrombin dynamics parameters	Unit	Parameter	Value	Norm.
Stationary amplitude of thrombin peak	AU/L	Ast	35,4	33,0-100,0
Rate of thrombin peak propagation	um/min	Vt	10,2	24,0-44,0

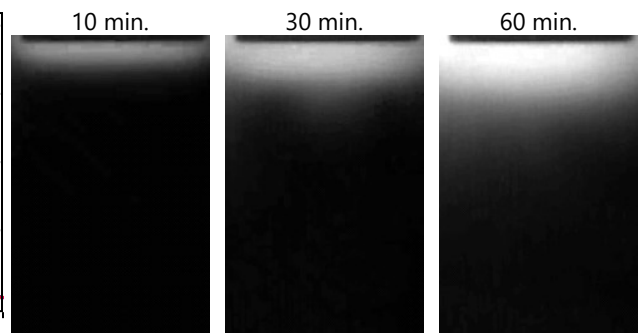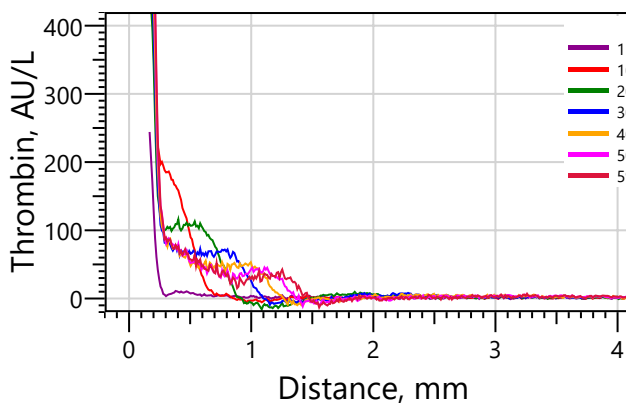

Comment:

Tech info:

ATTENTION: Research use only. Measurement results shouldn't be used for diagnostic purposes.

S/N: 000000, Operator: Operator, report created 29.03.2019 12:12

# Thrombodynamics Analyser


## Thrombodynamics-4D assay

24.08.2018 14:07

Measurement title: FIX Deficiency\_2% TD4D  
Plasma type: Fresh PFP  
Sample code: Example PLS #3

PLS

Activator thrombin generation (ATG) parameters	Unit	Parameter	Value	Norm.
Activator thrombin potential	AU*min/L	ETP_ATG	1371,3	1220,0-2170,0
ATG Maximum thrombin concentration	AU/L	Cmax_ATG	306,4	230,0-410,0
ATG Lag time	min	Lag_ATG	0,1	0,1-0,2
ATG Time to peak	min	Tmax_ATG	1,0	1,5-2,0

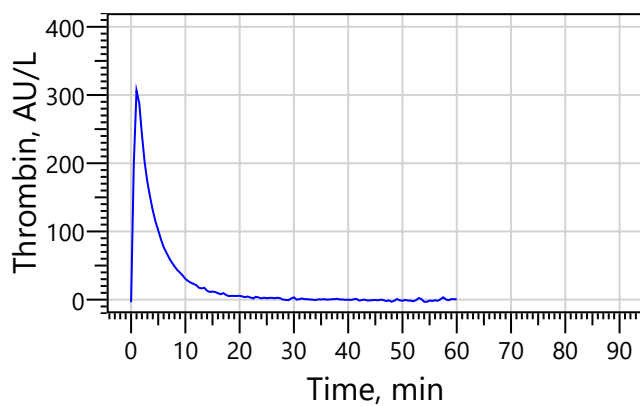

Comment:

Tech info:

ATTENTION: Research use only. Measurement results shouldn't be used for diagnostic purposes.

S/N: 000000, Operator: Operator, report created 29.03.2019 12:12



e0ba155c-f2e7-4e54-a182-ecf8711acfef