

Thrombodynamics Analyser

Thrombodynamics-4D assay



18.04.2018 15:28

Measurement title: Riva_0.3_um Effect TD4D
 Plasma type: Fresh PFP
 Sample code: Example PLS #4.3



PLS



Fibrin dynamics parameters	Unit	Parameter	Value	Norm.
Rate of clot growth	um/min	V	31,6	34,0-44,0
Lag time	min	Tlag	1,4	0,6-1,5
Initial rate of clot growth	um/min	Vi	63,4	59,0-69,0
Stationary rate of clot growth	um/min	Vst	31,6	34,0-44,0
Clot size at 30 min	um	CS	1332	1380-1640
Clot density	a.u.	D	24099	19500-34200
Spontaneous clotting	min	Tsp		30,0-

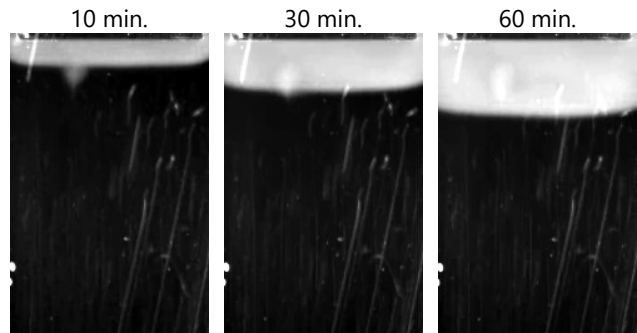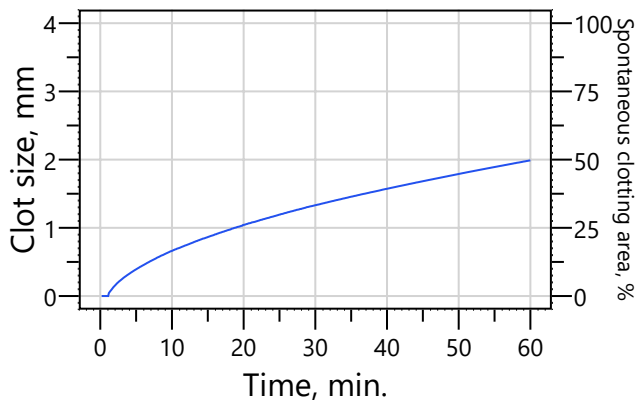

Thrombin dynamics parameters	Unit	Parameter	Value	Norm.
Stationary amplitude of thrombin peak	AU/L	Ast	32,2	33,0-100,0
Rate of thrombin peak propagation	um/min	Vt	18,2	24,0-44,0

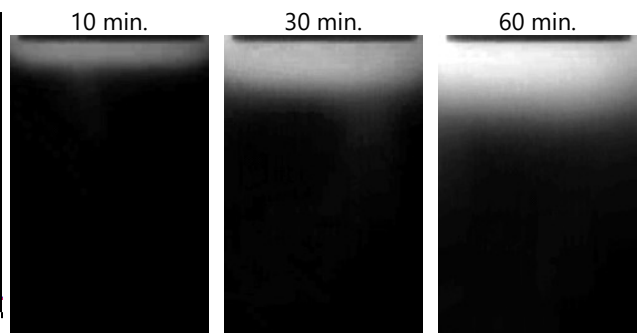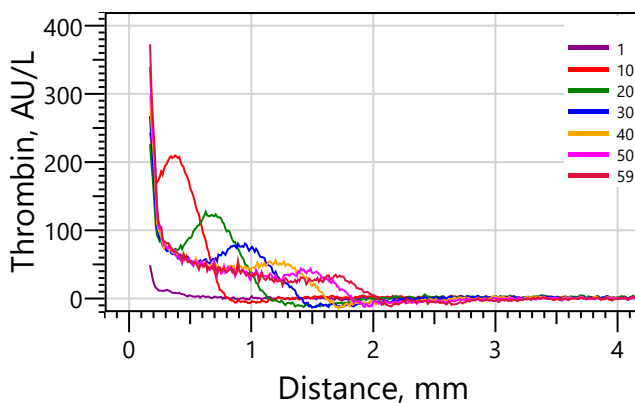

Comment: In-vitro spiking of control sample with direct inhibitor of FXa - rivaroxaban.

Tech info:

ATTENTION: Research use only. Measurement results shouldn't be used for diagnostic purposes.

S/N: 000000, Operator: Operator, report created 29.03.2019 12:12

Thrombodynamics Analyser


Thrombodynamics-4D assay

18.04.2018 15:28

Measurement title: Riva_0.3_um Effect TD4D
Plasma type: Fresh PFP
Sample code: Example PLS #4.3

PLS

Activator thrombin generation (ATG) parameters	Unit	Parameter	Value	Norm.
Activator thrombin potential	AU*min/L	ETP_ATG	1306,0	1220,0-2170,0
ATG Maximum thrombin concentration	AU/L	Cmax_ATG	211,1	230,0-410,0
ATG Lag time	min	Lag_ATG	0,3	0,1-0,2
ATG Time to peak	min	Tmax_ATG	2,0	1,5-2,0

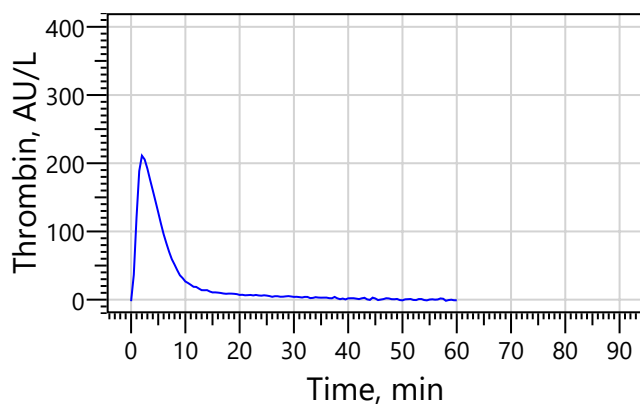

Comment: In-vitro spiking of control sample with direct inhibitor of FXa - rivaroxaban.

Tech info:

ATTENTION: Research use only. Measurement results shouldn't be used for diagnostic purposes.

S/N: 000000, Operator: Operator, report created 29.03.2019 12:12



1810c76d-3380-4b3c-9c81-a5cb98845c0b