

Thrombodynamics Analyser

Thrombodynamics assay



29.01.2018 10:57

Measurement title: Normal Coagulation + Hyperfibrinogenemia TD
 Plasma type: Fresh PFP
 Sample code: Example TDX #2

TDX



Fibrin dynamics parameters	Unit	Parameter	Value	Norm.
Rate of clot growth	um/min	V	25,4	20,0-29,0
Lag time	min	Tlag	1,0	0,6-1,5
Initial rate of clot growth	um/min	Vi	54,4	38,0-56,0
Stationary rate of clot growth	um/min	Vst	25,4	20,0-29,0
Clot size at 30 min	um	CS	1128	800-1200
Clot density	a.u.	D	34824	15000-32000
Spontaneous clotting	min	Tsp		30,0-

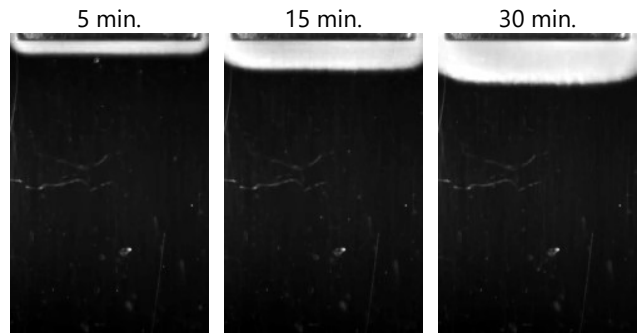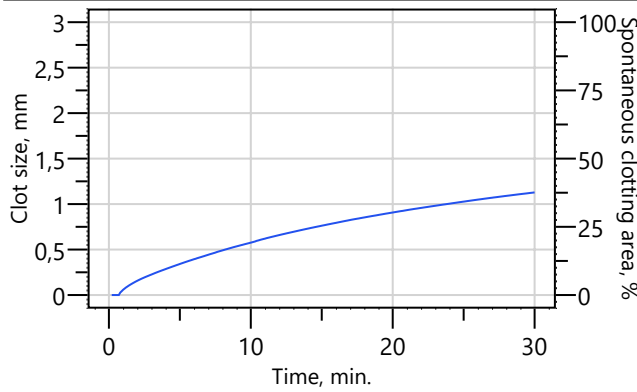

Comment:

Tech info:

ATTENTION: Research use only. Measurement results shouldn't be used for diagnostic purposes.

S/N: 000000, Operator: Operator, report created 29.03.2019 12:12