

Thrombodynamics Analyser



Thrombodynamics assay

30.09.2018 11:05

Measurement title: Before LMWH TD
Plasma type: Fresh PFP
Sample code: Example TDX #7.0

TDX

Fibrin dynamics parameters	Unit	Parameter	Value	Norm.
Rate of clot growth	um/min	V	36,2	20,0-29,0
Lag time	min	Tlag	0,9	0,6-1,5
Initial rate of clot growth	um/min	Vi	54,9	38,0-56,0
Stationary rate of clot growth	um/min	Vst	36,2	20,0-29,0
Clot size at 30 min	um	CS	1320	800-1200
Clot density	a.u.	D	27704	15000-32000
Spontaneous clotting	min	Tsp		30,0-

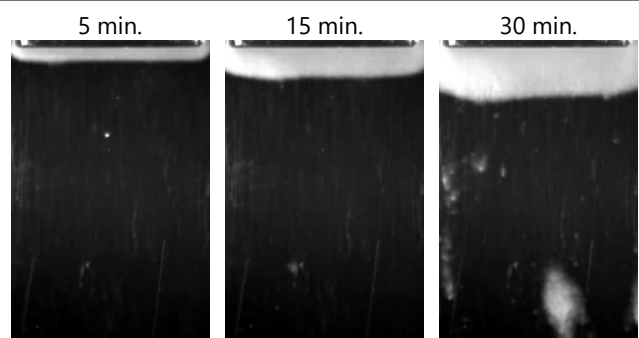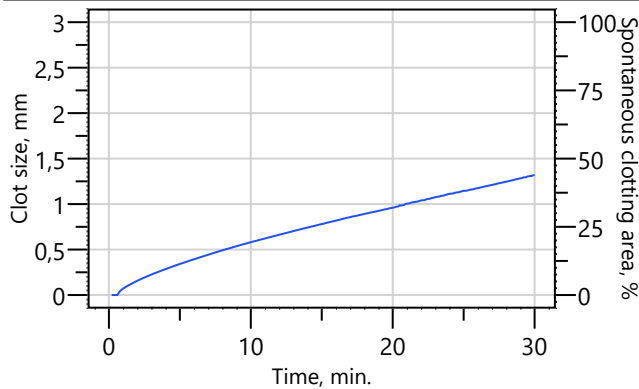

Comment: Hypercoagulation state is registred.

Tech info:

ATTENTION: Research use only. Measurement results shouldn't be used for diagnostic purposes.

S/N: 000000, Operator: Operator, report created 29.03.2019 12:12



dc4c2fbf-cd4e-4f1c-bc54-909f2efa7547