

Thrombodynamics Analyser



Thrombodynamics assay

12.10.2018 09:58

Measurement title: LMWH_tail TD
Plasma type: Fresh PFP
Sample code: Example TDX #7.2

TDX

Fibrin dynamics parameters	Unit	Parameter	Value	Norm.
Rate of clot growth	um/min	V	27,7	20,0-29,0
Lag time	min	Tlag	0,9	0,6-1,5
Initial rate of clot growth	um/min	Vi	48,6	38,0-56,0
Stationary rate of clot growth	um/min	Vst	27,7	20,0-29,0
Clot size at 30 min	um	CS	1098	800-1200
Clot density	a.u.	D	29179	15000-32000
Spontaneous clotting	min	Tsp		30,0-

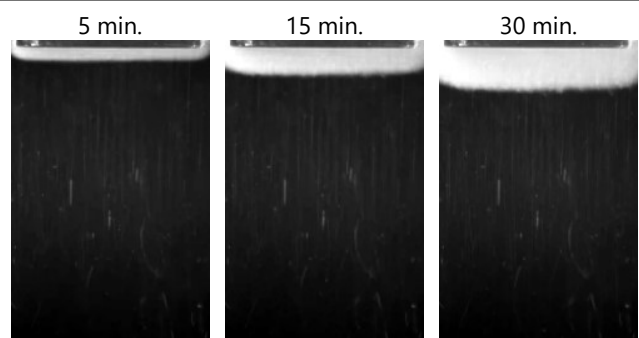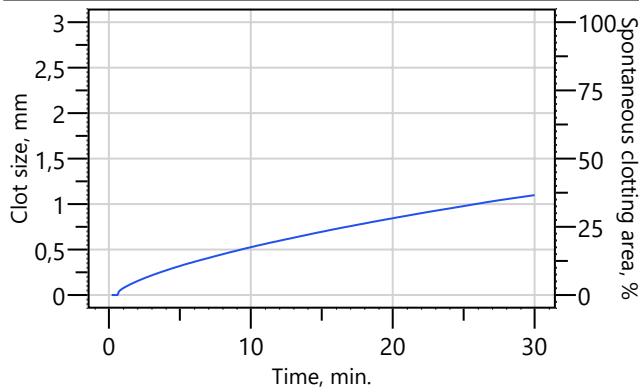

Comment: Measured (blood collection) 24h after 40mg/0.4 ml of enoxaparin.

Tech info:

ATTENTION: Research use only. Measurement results shouldn't be used for diagnostic purposes.

S/N: 000000, Operator: Operator, report created 29.03.2019 12:12



6293a38e-5f9f-491c-b481-6ffcc2b69055